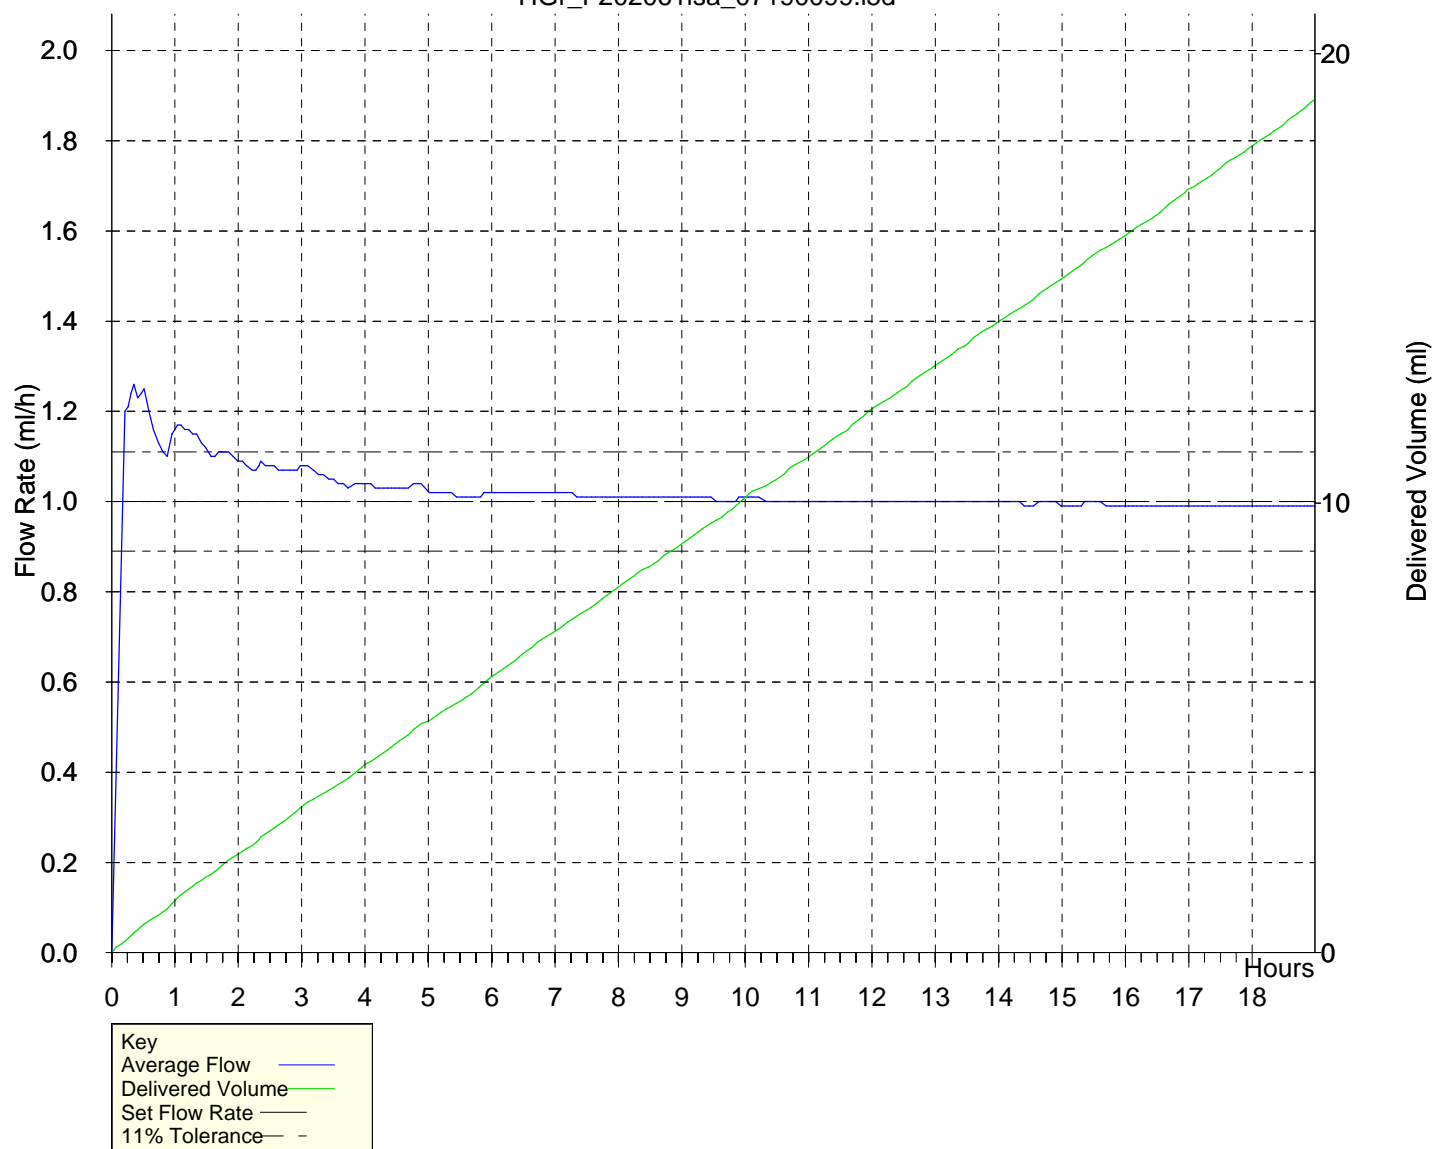


HGr_F202061isa_07190099.i5d

**Test Parameters**

Control Number essai
 Type of Test Flow
 Date Tested 10-Apr-2020
 Start Time 15:25:38
 Tested by PESTEL

Test Instrument

Fluke Biomedical IDA-5
 Infusion Device Analyzer
 Serial Number 4603553
 Version Ver 1.37
 Channel 1 S/N 07190099 Ver 1.05

Pump Details

Manufacturer ELECTROLAB
 Device Type (Model) Prototype 1
 Serial Number
 Location
 Comments

Set Values

Flow Rate 1.00 ml/h
 Total Volume 50.00 ml

Measured Values

Flow Rate 1.00 ml/h
 Total Volume 18.98 ml
 Total Test Time 18:59:20